

Title: Free Analyte Detection System
Inventor(s): Sales Amill et al.
Serial No. Not Yet Assigned
Atty Docket No. INL-048 (4643/86)
Atty/Agent: Ronda P. Moore
Express Mail Label No.: EL816798987US

如是者，人情之常也。故曰：「人情有所不能忍者。」

FIG. 1A




FIG 13

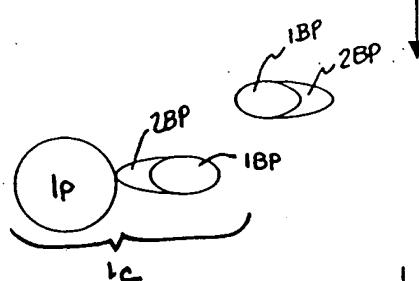


FIG. 1C







FIG. 2A

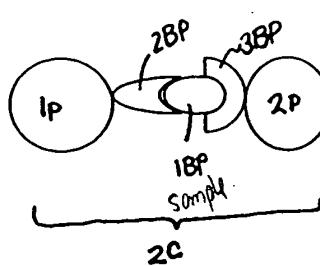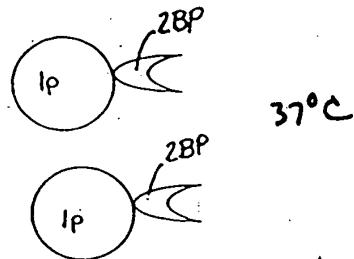

37°C




FIG. 2B





FIG. 2C

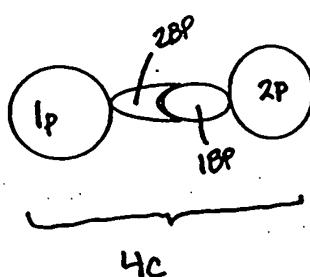

4C


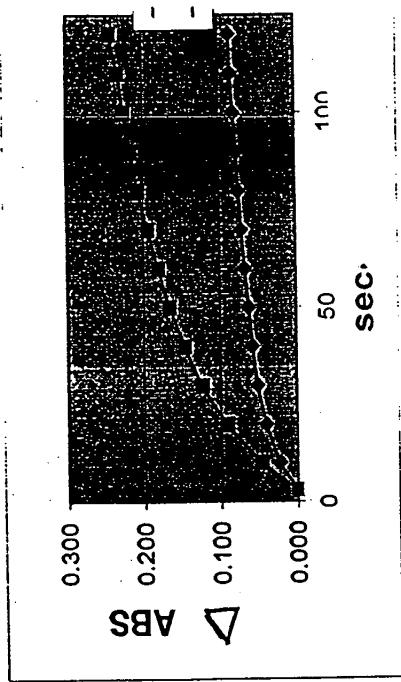


FIGURE 3

Title: Free-Amino Acide Detection System
Inventors: Sales Amill et al
Serial No. Not Yet Assigned
Amy Doctor No. INL-048 (4643/86)
Amy Ageent Round P. Moore
Amy Doctor No. IEL-048 (4643/86)
Express Mail Label No. E2816798987US

Figure 4

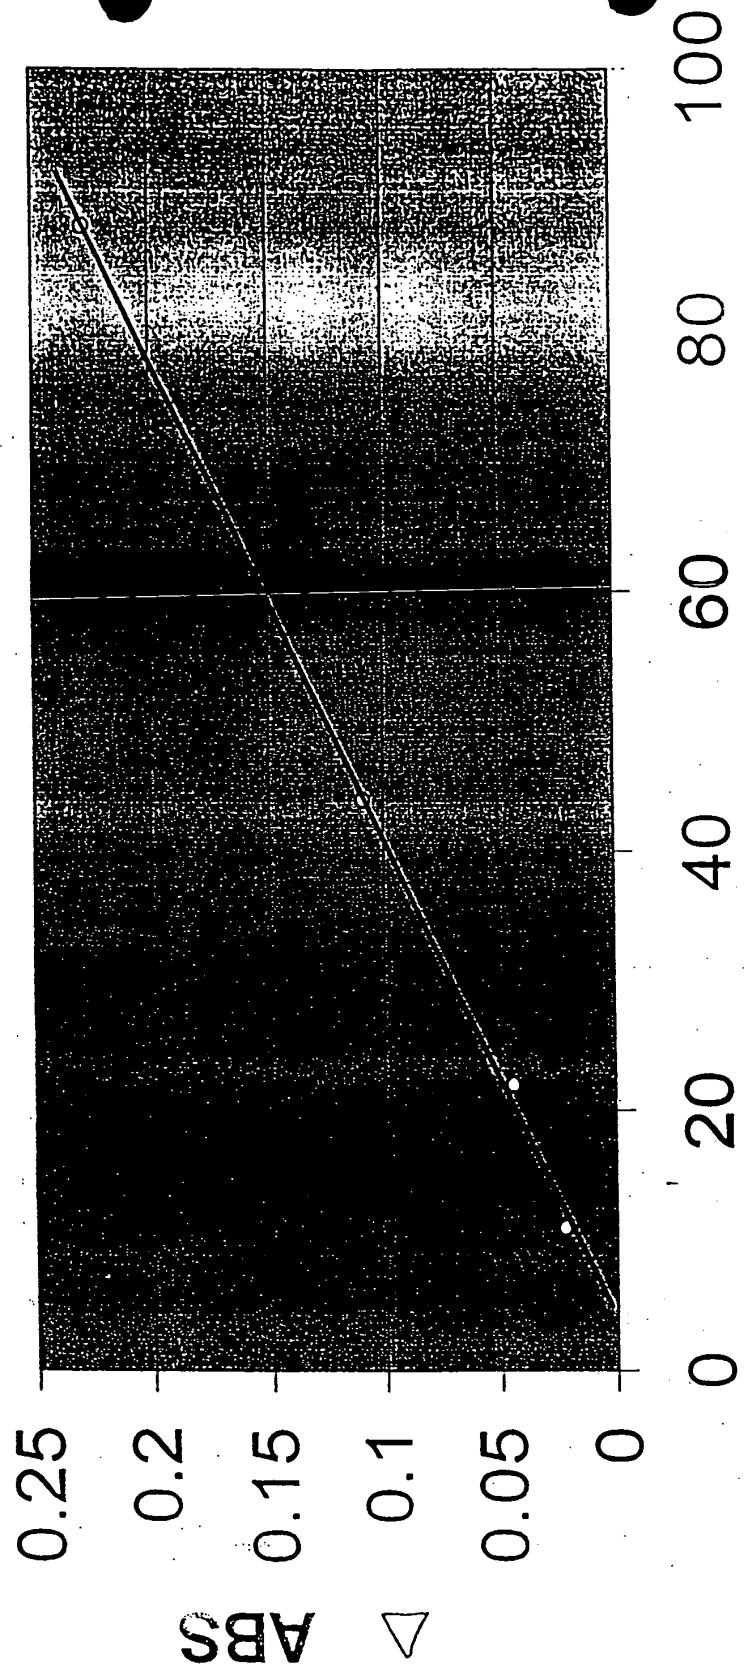

Title: Free Analyte Detection System
Inventor(s): Sales Amill et al
Serial No.: Not Yet Assigned
Artv/Decrter No.: INL-018 (466386)
Artv/Agent: Linda P. Moore
Express Mail Label No.: EL816798987US